

SurgiVet[®] Advisor[®] Vital Signs Monitor features SunTech Advantage NIBP module

Since January 2008, Smiths Medical PM Inc. has been incorporating the SunTech Advantage NIBP Module into the SurgiVet[®] Advisor[®] Vital Signs Monitor. SunTech Medical, Inc. is a leading global provider of blood pressure monitors and non-invasive blood pressure OEM technologies that has solely focused on blood pressure for more than 20 years.

While there are no formal veterinary regulatory requirements or guidelines, SunTech has recognized the need and obligation to study veterinary populations. Human monitors utilizing oscillometric technology do not have the sensitivity or range to be accurate in animals.

For a demonstration of the Advisor[®] Vital Signs Monitor, please contact a Smiths Medical sales manager, or call Smiths Medical customer service at 888-745-6562 (US only) or +1-262-513-8500.

SunTech has focused on the veterinary market and the unique requirements of taking blood pressure readings on patients unable to interact or communicate. The clinical environment is further complicated in the alert patient due to the stresses of being in an unfamiliar place surrounded by startling sounds and smells. Since animal types vary, structural, anatomical, physiological and pulse pressure properties further complicate accurate blood pressure monitoring, even in sedated/anesthetized patients. Their veterinary algorithm has been refined to accommodate these concerns and manage patient motion artifact thereby maximizing utility in both the awake and sedated patient.

Taking all these factors into consideration, SunTech has identified specific characteristics which are essential for designing an oscillometric blood pressure system for veterinary applications.

- Since animal types vary, systolic and diastolic pressures can be very high and extremely low. Accuracy is required throughout the expanded range.
- The BP system must be easy to use since the training and skill level of veterinary technicians vary.
- The BP monitor must be able to obtain accurate results on almost every attempt.
- Taking a reliable reading on the first attempt is crucial since an alert animal may become increasingly agitated.

To put the Advantage 2 Veterinary module to the test, a controlled trial was conducted at the North Carolina State University College of Veterinary Medicine. Their vet NIBP algorithm was compared against a Cardell Model 9402 NL monitor and a Critikon Dinamap Plus 9720 monitor on both dogs and cats. The reference device was an Ultrasonic Doppler Flow Detector Model 811-B. While it can be argued that Doppler does not provide a diastolic value, the technology is universally accepted in veterinary medicine to provide systolic values. A wide variety of animal subjects were used in this comparison to better replicate actual conditions in a veterinary clinic.

Methods

The data collection methodology included gathering pre and post Doppler measurements where oscillometric NIBP measurements were taken in between the pre and post Doppler measurements. The oscillometric NIBP measurements were performed simultaneously on contralateral limbs with the SunTech Advantage module on one and a competitive device on the other. Three simultaneous

measurements were done. Both the pre and post Doppler values were calculated by performing three sequential Doppler measurements which were averaged together.

All measurements were performed on both alert and sedated/anesthetized dogs and cats. In general, most dogs were anesthetized and most cats were awake. Animal conditions varied from healthy to critical to more closely replicate real conditions in a veterinary environment. The majority of animals had some sort of health issue ranging from dental prophylaxis to brain surgery. Subject (cat and dog) blood pressures included hypotensive, normotensive and hypertensive.

Weights and ages for cats varied from 1.3 to 10 kg (2.9 to 22.0 lb) and eight weeks to 17 years old. For dogs, weights were 8 to 44 kg (17.6 to 97 lb) and ages were one to 13 years old. A total of 29 cats and 48 dogs were involved in this comparison. The majority of subjects were included in the Cardell arm of the comparison (29 cats, 28 dogs). The remaining 20 dogs were included in the Critikon Dinamap comparison.

Since Doppler measurements only provide a systolic measurement, comparisons for diastolic, mean arterial pressure (MAP) and heart rate were not performed.



While accuracy is an important attribute in NIBP monitoring, reliability and consistency are particularly valuable in veterinary medicine. Operator confidence in being able to get needed results with the Advantage Model 2 Veterinary module can facilitate interventions in these traditionally difficult to manage patients.

Results:

SunTech – Cardell Systolic Accuracy Comparison		
Cats (n = 29)	Mean	Standard Dev
SunTech Advantage	-2.7	28.1
Cardell Monitor	15.5	34.5
Dogs (n = 28)		
SunTech Advantage	3.0	18.1
Cardell Monitor	4.7	21.4

SunTech – Dinamap Systolic Accuracy Comparison		
Dogs (n = 20)	Mean	Standard Dev
SunTech Advantage	1.1	11.7
Dinamap Monitor	5.0	20.8

Systolic comparisons with Doppler reference on cats and dogs

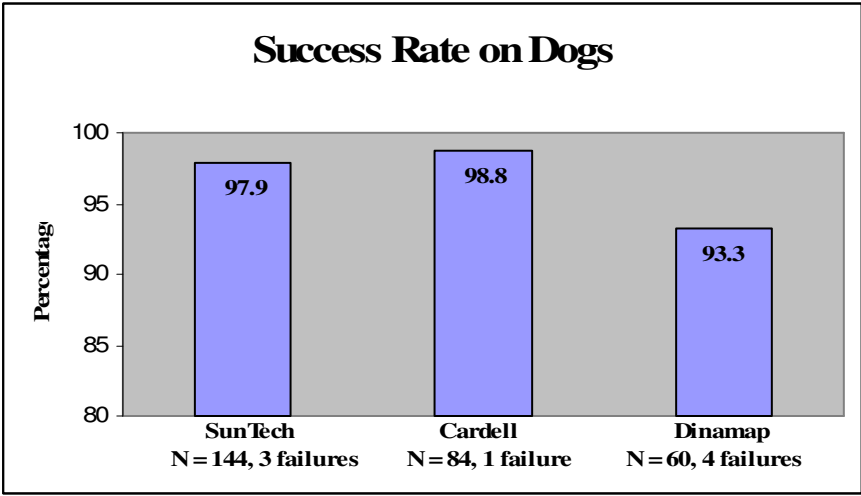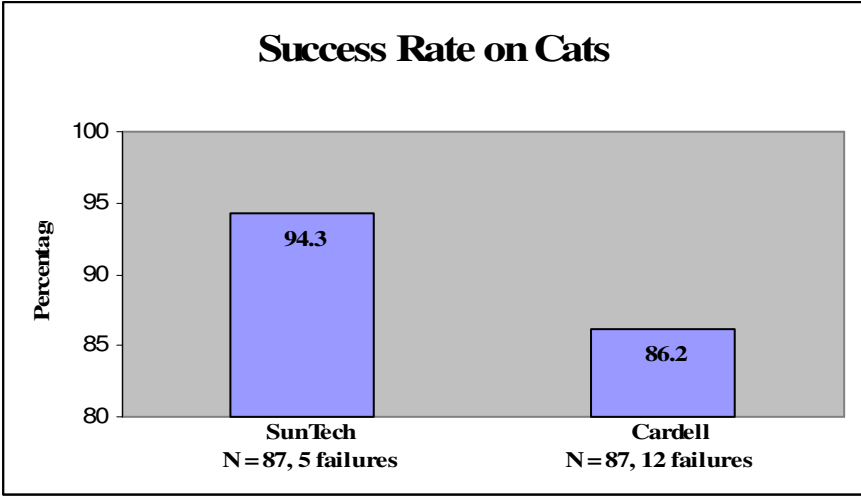

Oscillometric device success rates on cats and dogs